



Navigation

[UCBNE Home Page](#)
[Overview](#)
[Undergraduate](#)
[Graduate](#)
[News and Events](#)
[People](#)
[Research](#)
[Services](#)
[Careers](#)
[Class Schedule](#)
[Fall 2011 Class Schedule](#)
[Spring 2011 Class Schedule](#)
[NE Courses and Websites](#)
[create content](#)
[Public Forums](#)
[Colloquiums](#)
[ANS Berkeley Student Section](#)

Home

UCB Milk Sampling Results

[Back to Main UCB Air and Water Sampling Page](#)

The following are results for milk samples obtained from a Bay Area organic dairy where the farmers are encouraged to feed their cows local grass. We have detected I-131, Cs-134, and Cs-137 and are tracking their levels.

4/13/2011: Major revision note: *We just performed a major revision of our preliminary milk measurements. Our activity measurements for milk with a "best by" date after 4/4/2011 were accidentally calculated for the "best by" date itself, rather than an earlier date such as the purchase date. Since milk can be on the shelves starting almost 18 days before the "best by" date, our numbers after 4/4/2011 did not accurately reflect the maximum activity that the radioisotopes could have at the time of purchase. Incidentally, our first two milk measurements were not corrected at all and therefore reflect the activity at the time of measurement. The original numbers are at the bottom of the page for reference.*



*In order to make a valid comparison between all milk samples, we decided to correct all milk samples to represent the activity at their time of bottling -- this is 18 days before the "best by" date. This revision does not change the Cs-134 or Cs-137 numbers since they have long radioactive half-lives. The I-131 activity increases by factors of 2 to 5 because of its 8 day half-life. **Please note that though all I-131 activities have increased due to this revision, the levels are still very low -- one would have to consume at least 1,900 liters of milk to receive the same radiation dose as a cross-country airplane trip.***

In the table below the plot, we are providing two numbers for each of the isotopes. The first is a standard concentration unit of Becquerel per liter (Bq/L) which describes the number of particles decaying over the period of one second. For the general public, we have converted this number to an exposure dose per liter of milk consumed. The number in parentheses is the number of liters of milk that one would need to consume to equal the radiation exposure of a single round trip flight from San Francisco to Washington D.C. (0.05 mSv). For more information on how this equivalent dose is calculated, the details are here:

[How Effective Dose is Calculated](#)

Because the "best by" date on milk is approximately 17-19 days after the milk has been bottled, our milk sample with a date of 3/25 represents milk bottled on approximately 3/5. Since this is before the Fukushima crisis, we do not expect to see any fission product radioisotopes and do not see any within our sensitivity. Our first sample of milk showing any signs of radioisotopes has a date of 4/4, which means it was bottled around 3/18. This is approximately when the trace radioactive isotopes were first seen in the Bay Area.

The first two milk measurements were done with the same setup as the [Rainwater Collection Experiment](#), except that the milk is not distilled first before counting it with the germanium detector. The remaining measurements are being performed with a [mechanically-cooled germanium detector on loan from ORTEC and AMETEK](#). The new detector is larger than the previous detector, and we can fit almost an entire gallon of milk in the Marinelli beaker (previously, we could measure only one quart of milk). This leads to an improvement in overall sensitivity to radioactive isotopes.

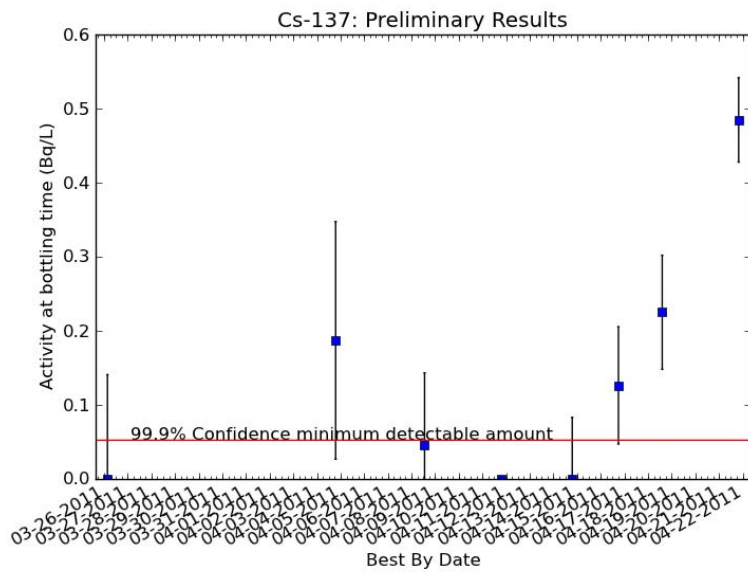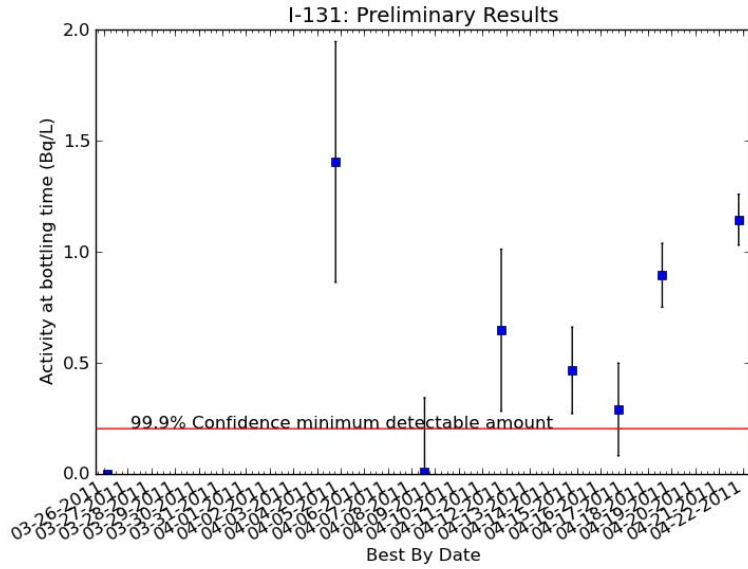

	I131	I132	Cs134	Cs137	Te132	Data
Best By Date	Bq/L (liters**)	Bq/L (liters**)	Bq/L (liters**)	Bq/L (liters**)	Bq/L (liters**)	
<i>Estimated Minimum Detectable Activity (MDA) for samples ending 4/4</i>	0.14	0.23	0.14	0.18	0.10	
3/25/2011	less than MDA	less than MDA	less than MDA	less than MDA	less than MDA	data
4/4/2011	1.40 ± 0.54 (1,900)	less than MDA	less than MDA	less than MDA	less than MDA	data
<i>Estimated Minimum Detectable Activity (MDA) for samples starting 4/8</i>	0.20		0.05		0.03	
4/8/2011	less than MDA	less than MDA	less than MDA	less than MDA	less than MDA	data
4/11/2011	0.65 ± 0.36 (4,200)	less than MDA	less than MDA	less than MDA	less than MDA	data
4/14/2011	0.47 ± 0.19 (5,800)	less than MDA	0.11 ± 0.04 (22,000)	less than MDA	less than MDA	data

4/16/2011	less than MDA	less than MDA	less than MDA	0.13 ± 0.08 (21,000)	less than MDA	data
4/18/2011	0.89 ± 0.14 (3,000)	less than MDA	0.10 ± 0.04 (24,000)	0.22 ± 0.08 (12,000)	less than MDA	data
4/21/2011	1.14 ± 0.11 (2,400)	less than MDA	0.37 ± 0.04 (6,500)	0.48 ± 0.06 (5,600)	less than MDA	data

** The number in parentheses is the number of liters of milk that one would need to consume to equal the radiation exposure of a single round trip flight from San Francisco to Washington D.C. (0.05 mSv). To see how we calculate these numbers, please visit [our explanation of the equivalent dose calculation](#).

Original Data (pre-4/13/2011):

	I131	I132	Cs134	Cs137	Te132	Data
Best By Date	Bq/L (liters**)	Bq/L (liters**)	Bq/L (liters**)	Bq/L (liters**)	Bq/L (liters**)	
<i>Estimated Minimum Detectable Activity (MDA) for samples ending 4/4</i>	0.14	0.23	0.14	0.18	0.10	
3/25/2011	less than MDA	less than MDA	less than MDA	less than MDA	less than MDA	data
4/4/2011	0.70 ± 0.27 (3,800)	less than MDA	less than MDA	less than MDA	less than MDA	data
<i>Estimated Minimum Detectable Activity (MDA) for samples starting 4/8</i>	0.04		0.05		0.03	
4/8/2011	less than MDA	less than MDA	less than MDA	less than MDA	less than MDA	data
4/11/2011	0.14 ± 0.08 (18,900)	less than MDA	less than MDA	less than MDA	less than MDA	data
4/14/2011	0.10 ± 0.04 (26,300)	less than MDA	0.11 ± 0.04 (22,100)	less than MDA	less than MDA	data
4/16/2011 4/18/2011	0.22 ± 0.04 (12,200)	less than MDA	0.10 ± 0.04 (24,000)	0.22 ± 0.08 (12,000)	less than MDA	data

UC Berkeley • College of Engineering • American Nuclear Society, UCB, Student Section
 4155 Etcheverry Hall, MC 1730, Berkeley, CA 94720 • FAX 510-643-9685
 • Main Office: Maria Drezgich, 510-642-4077
 • This site is designed by Bill King, 2008, All Rights Reserved
 Campanile photo courtesy of Andrew P. Keating <http://andrewpkeating.com>